Ringbio



Ring Biotechnology Co Ltd

info@ringbio.com

In each kit


- 50 test cards in foil pouch
- 50 plastic pipet
- Kit instruction

Sample


- Fresh pig urine from sows 22-32 days after AI or mating
- Bring sample to room temp. before testing



How to run the pig pregnancy test kit

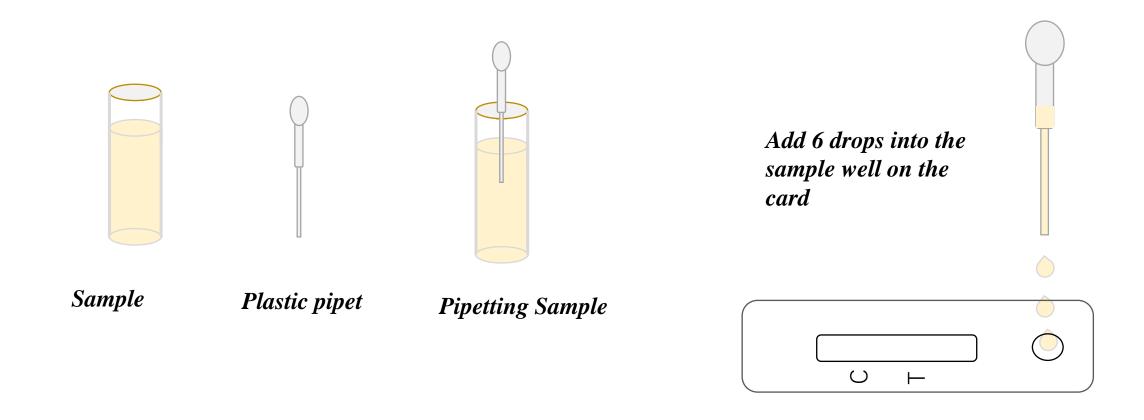

Sample flow on the card from sample well to test zone

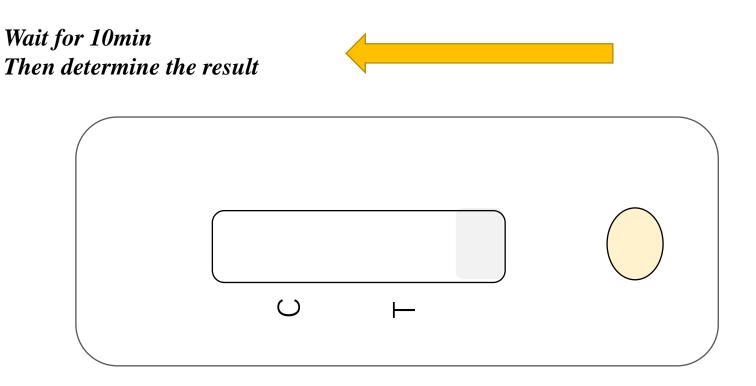


Determine the result

Compare the color of Line C & Line T

Positive: C >= T (including No Line T)

Negative: C < T

Invalid: No Line C

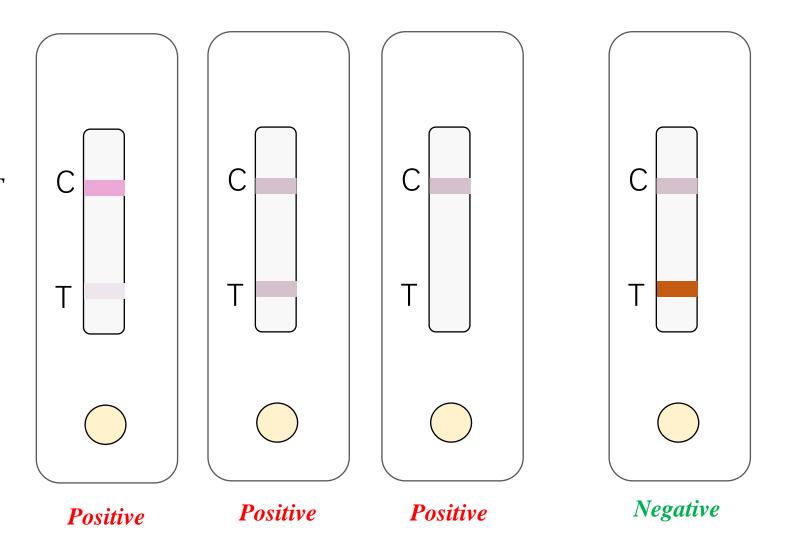

Caution

- This kit is only for sows after breeding or AI,.
- This kit can not be used with boar or open pig urine.
- This kit can not detect pig pregnancy 48-62days after breeding or AI due to the hormone concentration change.

Ringbio

Contact us

www.ringbio.com

info@ringbio.com